



HeartSine samaritan® PAD
SAM 500P Trainer
model TRN-500-1
User Manual



HeartSine samaritan PAD 500P Trainer with CPR Advisor™

This User Manual provides instructions on how to operate the HeartSine samaritan PAD 500P Trainer.

The HeartSine samaritan PAD 500P Trainer is a non-medical device intended to be used for the training of emergency responders in the proper use of the HeartSine samaritan PAD 500P automated external defibrillator. The Trainer has no therapeutic capabilities and must not be used in real life rescue situations.



IMPORTANT: *In order to avoid confusion in the event of a real life rescue, do not store or leave the Trainer near the HeartSine samaritan PAD 500P automated external defibrillator.*

To allow quick and easy identification the HeartSine samaritan PAD 500P Trainer incorporates a yellow front user interface membrane whereas the HeartSine samaritan PAD 500P automated external defibrillator has a navy blue/black front membrane.

HeartSine recommends that responders who may use one of its defibrillators should be trained in Cardiopulmonary Resuscitation with defibrillator use (CPR-D). The HeartSine samaritan PAD 500P Trainer is intended to be used by approved CPR-D training providers for this purpose.

The HeartSine samaritan PAD 500P Trainer is factory configured to operate in accordance with the joint American Heart Association/European Resuscitation Council 2015 guidelines for CPR. The device comes with six preprogrammed scenarios based on these guidelines.

Should the CPR guidelines change, software will be available to upgrade the HeartSine samaritan PAD 500P Trainer to comply. Please contact your HeartSine authorized distributor or HeartSine Technologies direct.

Once turned on the HeartSine samaritan PAD 500P Trainer will play audible voice prompts with accompanying visual indicators. The HeartSine samaritan PAD 500P Trainer may also be controlled using the accompanying Remote Control included with the device.

Please contact your authorized HeartSine distributor for a list of replacement accessories.

Preparing the HeartSine samaritan PAD 500P Trainer for Use

- 1) Ensure that the HeartSine samaritan PAD 500P Trainer is fully charged (see the Charging section of this manual).
- 2) Place the HeartSine samaritan PAD 500P Trainer and the Trainer-Pak™ on a flat surface. Push the Trainer-Pak into the opening of the HeartSine samaritan PAD 500P Trainer and listen for a “click” sound to ensure that it is properly inserted.
- 3) Place the batteries supplied with your Trainer into the HeartSine samaritan PAD 500P Remote Control.

 *Do not press any buttons whilst inserting the Remote Control batteries as this will reset the Remote Control ID.*

- 4) Press the On/Off button on the HeartSine samaritan PAD 500P Trainer and listen to the voice prompts to ensure that the unit is functioning.
- 5) If the HeartSine samaritan PAD 500P Trainer has insufficient charge, it will not function correctly. When switched on, the Status Indicator will flash red to indicate that charging is required. If the battery is fully depleted the device will not power on at all. For full charging instructions see the Charging section of this manual.

Turning on and off the HeartSine samaritan PAD 500P Trainer

To turn on the HeartSine samaritan PAD 500P Trainer press the green On/Off button.



 *By default the Trainer will function in the last scenario setting used.*

To turn off the HeartSine samaritan PAD 500P Trainer press the On/Off button again.

Once the HeartSine samaritan PAD 500P Trainer has been turned on, it may be turned off using the accompanying Remote Control. To turn the Trainer off press the Off button (red button) on the Remote Control.

 *When turned on the HeartSine samaritan PAD 500P Trainer will automatically turn Off after fifteen minutes if the device is not being used.*

HeartSine samaritan PAD 500P Trainer

HeartSine samaritan PAD 500P Trainer



- A Data Port
- B Battery Charge Status LED
- C Status Indicator
- D Shock Button
- E Do Not Touch Indicator
- F Speaker
- G Trainer-Pak Cartridge
- H On/Off Button
- I Safe To Touch Indicator
- J CPR Indicator
- K Pads Placement Indicator
- L Action Arrows



On/Off button

Press this button to turn the device on and off. (If pressed whilst a shock is advised, a warning is issued "Warning, Off button pressed"; the device will not power Off unless you press the button again within three seconds.)



Pads placement indicator

The action arrows around this icon will flash to instruct the user that the HeartSine samaritan PAD 500P pads should be attached to the patient as indicated.



Safe to touch indicator

It is safe to touch the patient when the action arrows around this icon are flashing. You may perform CPR or check the patient.



Status Indicator

Flashing green - Trainer is ready for use
Flashing red - Trainer requires charging



Action arrows

The action arrows around an icon will flash to indicate the actions that the user should be performing.



Do not touch indicator

Do not touch the patient when the action arrows around this icon are flashing. The PAD 500P may be analyzing the patient's heart rhythm or preparing to deliver a shock.



Shock button

Press this button to simulate delivery of a therapeutic shock.



CPR indicator

This is an array of lights which provide a graduated indication of the force being applied during CPR compressions. When green lights illuminate the compressions are considered to be of adequate force.

Managing the Electrodes


Using the Electrodes

The training scenarios include audible prompts to remove the electrodes from the Trainer-Pak and to position the electrode pads as indicated. Follow the steps below when prompted to do so.

- 1) Pull the green tab to open the Trainer-Pak cartridge and fully extend the electrode cables.
- 2) Peel the electrode pads from their protective liners.
- 3) Position the electrode pads as indicated by the Pads Placement Indicator; sternum and apex electrode pads are clearly identified on their respective pads.
- 4) Press the pads firmly to ensure that proper contact is made.

Rewinding the Electrodes after Use

- 1) Re-attach the protective liners to the electrode pads, or replace with new pads.
- 2) Fold the pads together so that the liner is on the outside.
- 3) Let the electrodes hang from the device and use the handle in the blue coil mechanism to fully rewind the electrodes:

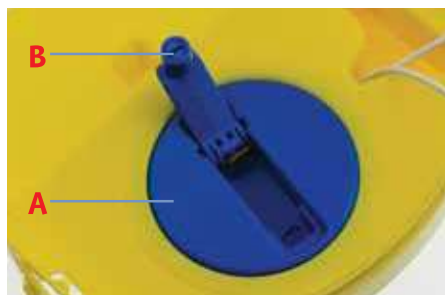

A Coil Mechanism

B Coil Handle

- 4) Place the pads on top of the Trainer-Pak cartridge, ensuring that the wires are beneath the pads.
- 5) Close the Trainer-Pak cartridge by sliding the yellow tray into place.


The Remote Control

HeartSine samaritan PAD 500P Trainer Remote Control



Turning off the Trainer

The Remote Control can be used to turn off the HeartSine samaritan PAD 500P Trainer. To turn the Trainer off press the red button on the Remote Control.




Changing the Volume

There are four volume settings available on the HeartSine samaritan PAD 500P Trainer. The volume control buttons are to the left of the Off button on the Remote Control. To increase the volume press the '+' button and to decrease the volume press the '-' button.



Pausing the Trainer

During training the HeartSine samaritan PAD 500P Trainer may be paused. To pause the Trainer press the Pause button (||). The Trainer will remain paused until the Pause button is pressed again at which point it will continue to play the scenario selected.



Changing the Scenario

The HeartSine samaritan PAD 500P Trainer comes with six preprogrammed training scenarios. (For details of the scenarios see the training scenarios section of this manual.) The scenario may be changed by pressing the appropriate number button on the Remote Control i.e. pressing '3' will select training scenario three.

Once the scenario has been changed the device will operate as detailed in the scenarios section. The device will remain in this scenario until a new scenario is selected.

Preprogrammed Training Scenarios

The HeartSine samaritan PAD 500P Trainer has six preprogrammed training scenarios to choose from. All preprogrammed scenarios are based on AHA/ERC 2015 guidelines. Details of the preprogrammed scenarios are given below.

Scenario 1

1. Setup mode - "Call for Medical assistance", "Pull green tab", etc
2. User intervention - "Pads" button to be pressed to confirm electrodes placed
3. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
4. Shock advised - User to press the shock button
5. CPR mode - User to apply CPR with advisory as required
6. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
7. No shock advised
8. CPR mode - User to apply CPR with advisory as required
9. Repeat - Steps 6 to 8 repeated until 'On/Off' button is pressed

Scenario 2

1. Setup mode - "Call for Medical assistance", "Pull green tab", etc
2. User intervention - "Pads" button to be pressed to confirm electrodes placed
3. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
4. No shock advised
5. CPR mode - User to apply CPR with advisory as required
6. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
7. Shock advised - User to press the shock button
8. CPR mode - User to apply CPR with advisory as required
9. Repeat - Steps 6 to 8 repeated until 'On/Off' button is pressed

Scenario 3

1. Electrodes - Device assumes the electrodes are already attached
2. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
3. Check Pads - "Check Pads"
4. User intervention - "Pads" button to be pressed to confirm electrodes placed
5. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
6. Shock advised - User to press the shock button
7. CPR mode - User to apply CPR with advisory as required
8. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
9. No shock advised
10. CPR mode - User to apply CPR with advisory as required
11. Repeat - Steps 3 to 10 repeated until 'On/Off' button is pressed

Preprogrammed Training Scenarios

Scenario 4

1. Electrodes - Device assumes electrodes are already attached
2. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
3. Shock advised - User to press the shock button
4. CPR mode - User to apply CPR with advisory as required
5. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
6. Shock advised - User to press the shock button
7. CPR mode - User to apply CPR with advisory as required
8. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
9. No shock advised
10. CPR mode - User to apply CPR with advisory as required
11. Repeat - Steps 5 to 10 repeated until 'On/Off' button is pressed

Scenario 5

Scenario 5 is the same as Scenario 1 with the addition of audible indications of when to perform rescue breaths during CPR mode.

1. Setup mode - "Call for Medical assistance", "Pull green tab", etc
2. User intervention - "Pads" button to be pressed to confirm electrodes placed
3. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
4. Shock advised - User to press the shock button
5. CPR mode - User to apply CPR with advisory as required; this includes an audible indication of when to perform rescue breaths - the metronome changes from a "beep" to a "tick" for the duration of ten compressions.
6. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
7. No shock advised
8. CPR mode - User to apply CPR with advisory as required; this includes an audible indication of when to perform rescue breaths - the metronome changes from a "beep" to a "tick" for the duration of ten compressions.
9. Repeat - Steps 6 to 8 repeated until 'On/Off' button is pressed

Scenario 6

Scenario 6 is the same as Scenario 2 with the addition of audible indications of when to perform rescue breaths during CPR mode.

1. Setup mode - "Call for Medical assistance", "Pull green tab", etc
2. User intervention - "Pads" button to be pressed to confirm electrodes placed
3. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
4. No shock advised
5. CPR mode - User to apply CPR with advisory as required; this includes an audible indication of when to perform rescue breaths - the metronome changes from a "beep" to a "tick" for the duration of ten compressions.
6. Monitor mode - "Assessing heart rhythm", "Do not touch the patient", etc
7. Shock advised - User to press the shock button
8. CPR mode - User to apply CPR with advisory as required; this includes an audible indication of when to perform rescue breaths - the metronome changes from a "beep" to a "tick" for the duration of ten compressions.
9. Repeat - Steps 6 to 8 repeated until 'On/Off' button is pressed

Manual Control of the HeartSine samaritan PAD 500P Trainer

The Remote Control allows Training providers to control the scenario manually. When turned on the HeartSine samaritan PAD 500P Trainer will operate as detailed in the training scenarios listed. Training providers can override this by pressing the 'Shock required', 'No Shock required' or 'Attach Electrode Pads' button.



Shock Required

Pressing the 'Shock required' button will cause the HeartSine samaritan PAD 500P Trainer to override the selected training scenario and simulate a shockable rhythm. Each subsequent analysis period will advise a shock to be delivered until either the Trainer is turned off or the 'No Shock required' button on the Remote Control is pressed.



No Shock Required

Pressing the 'No Shock required' button will cause the HeartSine samaritan PAD 500P Trainer to override the selected training scenario and simulate a non-shockable rhythm. Each subsequent analysis period will advise no shock to be delivered until either the Trainer is turned off or the 'Shock required' button on the Remote Control is pressed.



Attach Electrode Pads

If the 'Attach Electrode Pads' button is pressed the Trainer will play the 'Attach the electrodes' prompts during the analysis period of operation. The Trainer will continue to play 'Attach the electrodes' prompts until the 'Attach Electrode Pads' button is pressed again.

HeartSine samaritan PAD with CPR Advisor model 500P

The HeartSine samaritan PAD 500P automated external defibrillator incorporates a CPR feedback module called 'CPR Advisor'. The HeartSine samaritan PAD 500P uses the CPR Advisor function to provide simple feedback on the quality of the CPR being provided by rescuers. If appropriate the rescuer will be prompted to push harder until the compressions being provided are of sufficient force.

If the compressions are considered to be of sufficient force the CPR Advisor will then analyze the rate that compressions are being performed. The rescuer will be prompted to push faster or slower as appropriate.

If the CPR being provided is of sufficient force and rate the HeartSine samaritan PAD 500P will play a 'Good compressions' prompt.

All audible prompts are accompanied by visual prompts on the CPR indicator icon.

CPR Advisor Training Module

CPR Advisor Training

Training providers can simulate the CPR Advisor function on the HeartSine samaritan PAD 500P Trainer by using the Remote Control. Training providers should observe the CPR being provided by the rescuers being trained and based on observations press the appropriate button.

The HeartSine samaritan PAD 500P Trainer will initially assume correct compressions are being performed and play the audible prompt:



The CPR control buttons are at the bottom of the Remote Control. The buttons to the left are used to indicate the rate at which the trainee is performing compressions and the buttons to the right are used to indicate the force at which compressions are being delivered.

Compression Rate

Fast Compressions

Correct Rate

Slow Compressions



Compression Force

Begin CPR / No Compressions

Good Force

Insufficient Force


Compression Force

The HeartSine samaritan PAD 500P Trainer can mimic the CPR Advisor function on the HeartSine samaritan PAD 500P defibrillator.



CPR not started

If the trainee has not started to perform CPR press the 'No compressions' button. The HeartSine samaritan PAD 500P Trainer will play the audible prompt:



The 'CPR indicator' on the HeartSine samaritan PAD 500P Trainer has a single flashing orange light as shown. The trainee should begin CPR immediately.

CPR Advisor Training Module



Compressions not Hard Enough

If the trainee has started to perform CPR but they are of insufficient force, press the Insufficient Force button. The HeartSine samaritan PAD 500P Trainer will play the audible prompt:



"Push Harder"



The 'CPR indicator' on the HeartSine samaritan PAD 500P Trainer will flash yellow as shown. The trainee should be prompted to push harder.



Good Compression Force

If the trainee is performing compressions of sufficient depth press the 'Good Force' button. The CPR indicator icon will now flash all lights (yellow and green) as shown.



The HeartSine samaritan PAD 500P Trainer will no longer issue messages referring to the force with which the compressions are being given:



"Good Compressions"

Compression Rate

The HeartSine samaritan PAD 500P Trainer can mimic the CPR Advisor function on the HeartSine samaritan PAD 500P defibrillator. The following are instructions on how to simulate rate of compressions.



Compressions Too Slow

If the trainee is performing compressions too slowly press the 'Slow Compressions' button. The HeartSine samaritan PAD 500P Trainer will play the prompt:



"Push Faster"



Compressions Too Fast

If the trainee is performing compressions too quickly press the 'Fast Compressions' button. The HeartSine samaritan PAD 500P Trainer will play the prompt:



"Push Slower"



Compressions Correct Rate

If the trainee is performing compressions at the correct rate press the 'Correct Rate' button. The HeartSine samaritan PAD 500P Trainer will play the good compressions prompt.

Maintenance

HeartSine samaritan PAD 500P Trainer Battery Management

The HeartSine samaritan PAD 500P Trainer contains a rechargeable battery. It is recommended that you ensure the HeartSine samaritan PAD 500P Trainer is fully charged prior to commencing training activities.

When fully charged the HeartSine samaritan PAD 500P Trainer will give you approximately seven hours of usage before it needs to be recharged.

The HeartSine samaritan PAD 500P Trainer will monitor the capacity of the battery as it approaches depletion. A minimum of one hour prior to the battery becoming depleted the Trainer will play the following message:

 "Warning. Low battery"

If this warning is heard you may continue to use your HeartSine samaritan PAD 500P Trainer for a limited period of time. If the battery becomes completely depleted the Trainer device will shut itself down. At this point the Trainer should be recharged.

Charging and Recharging the HeartSine samaritan PAD 500P Trainer

To safely charge or recharge the HeartSine samaritan PAD 500P Trainer follow the instructions given below.

- 1) Insert the charger adaptor into the socket on the side of the HeartSine samaritan PAD 500P Trainer. Ensure that the adaptor is fully inserted.
- 2) Plug the charger into the mains electricity supply.
- 3) Leave the Trainer to charge. The Battery Charge Status LED (located beside the socket) will be red when fast charging and will flash when charging is almost complete. Once charging is complete the LED will switch off. To charge a depleted HeartSine samaritan PAD 500P Trainer will take a maximum of six hours.
- 4) Remove the adaptor from the HeartSine samaritan PAD 500P Trainer. Turn on the Trainer to ensure that the device is working.

If the HeartSine samaritan PAD 500P Trainer is switched on during charging the charger should be switched off then on again to restart fast charging.

The HeartSine samaritan PAD 500P Trainer must only be charged with the charger supplied with it. Use of any other charging device will nullify the warranty and may result in damage to the HeartSine samaritan PAD 500P Trainer.

The HeartSine samaritan PAD 500P Trainer and charger are designed for indoor use only. Do not use in wet or damp environments.

There are no user serviceable parts inside your HeartSine samaritan PAD 500P Trainer, Trainer-Pak or charger. These products should not be opened. In the unlikely event of a malfunction, please contact your distributor immediately.

Maintenance

Remote Control Batteries

The HeartSine samaritan PAD 500P Trainer Remote Control contains a low battery warning indicator. If this indicator flashes red two times after a button on the Remote Control is pressed it is an indication that the batteries within the Remote Control need to be replaced.

The Remote Control uses two standard AAA batteries.

The batteries can be accessed by removing the battery cover at the back of the Remote Control.



Inserting the batteries into the Remote Control whilst pressing the Off button will cause the Remote Control to enter pairing mode and take a new transmission ID. This will be different to that previously stored on the Trainer. If this occurs accidentally it will be necessary to complete the pairing procedure in full to pair the Remote Control with the HeartSine samaritan PAD 500P Trainer again. Normal battery replacement does not cause a problem since pairing is only initiated when the Off button is also held down.

HeartSine samaritan PAD 500P Trainer Configuration Tool

The HeartSine samaritan PAD 500P Trainer configuration tool is software that can be downloaded for free from the HeartSine website (www.heartsine.com). This software allows you to upgrade your Trainer. The following options are available.

Language

The HeartSine samaritan PAD 500P Trainer can be reprogrammed to operate with audible prompts in any one of a selection of languages. Download the current HeartSine samaritan PAD 500P Trainer configuration tool user manual from the HeartSine website for instructions on how to do this.

Pairing a Remote Control with the HeartSine samaritan PAD 500P Trainer

Each HeartSine samaritan PAD 500P Trainer has a specific Remote Control to operate it. This is to allow multiple devices to be used in close vicinity without interference. In the unlikely event that your Remote Control no longer operates with your Trainer it may need to be paired with your Trainer again.

The HeartSine samaritan PAD 500P Trainer Configuration Tool can be used to pair a Remote Control with your Trainer. Full instructions are contained within the accompanying user manual.

Device Identifications

Each HeartSine samaritan PAD 500P Trainer is given an identification number between 001 and 255 during manufacture. The Remote Control for each Trainer is then given the same identification number. In the unlikely event that two devices with the same ID number are being used at the same time use the HeartSine samaritan PAD 500P Trainer Configuration Tool to assign new numbers to the devices. It will be necessary to pair the device with its Remote Control after assigning a new ID number.

CPR Guidelines 2015

The following is a brief overview of the fundamentals of CPR for lay rescuers as advised by both the American Heart Association (AHA) and the European Resuscitation Council (ERC) in their 2015 published Guidelines for CPR and ECC. This is intended only as a quick reference for trained CPR providers. HeartSine recommend that all potential users of the HeartSine samaritan PAD 500P are trained by a competent training organization in both the use of CPR and HeartSine samaritan PAD 500P, prior to placing a HeartSine samaritan PAD 500P into service. Should the Guidelines change, software will be available to upgrade the HeartSine samaritan PAD 500P to comply. Please contact your HeartSine authorized distributor or HeartSine Technologies direct.


CALL Emergency Services
(119/999/911 etc.).
Send for an AED.
Person not responsive?
Address person and shake on
shoulder. Call Emergency Services.



Watch, feel, listen.
Open the airway, check for
breathing.




**Perform CPR following the latest
AHA or ERC guidelines.**
Perform CPR until an AED is available
OR arrival of emergency physician.
Engage other people to help you and
alternate CPR.



If available use an AED.

**Continue CPR until Emergency Services
arrive. Alternate with second person
after one cycle or 2 minutes.**

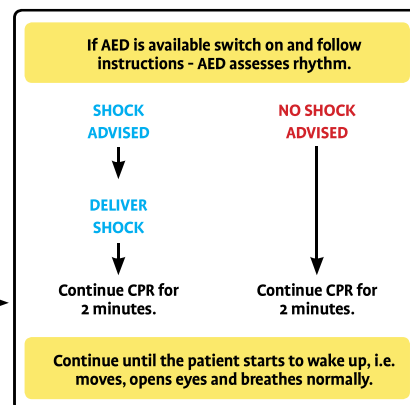

HeartSine samaritan PAD 500P Trainer

Disposal Instructions

The HeartSine samaritan PAD 500P Trainer is a reusable device. If maintained in accordance with the instructions in this manual it has a warranty period of two years from the date of manufacture.

If you wish to dispose of the HeartSine samaritan PAD 500P Trainer unit, it should be disposed of at an appropriate recycling facility according to national, state and local requirements. Alternatively return the unit to your local distributor or HeartSine Technologies for disposal.

Disposal within the European Union:

Do not dispose of the HeartSine samaritan PAD 500P Trainer unit as unsorted municipal waste: keep the HeartSine samaritan PAD 500P Trainer separate, to be reused or recycled in accordance with Directive 2002/96/EEC of the European Parliament and the Council of the European Union on Waste Electronic and Electrical Equipment (WEEE), or return to your local distributor or HeartSine Technologies for disposal.

Warranty Exclusion

HeartSine Technologies or the authorized distributors are not obliged to carry out service/repairs under warranty if:

- a. Unauthorized modifications have been made to the device.
- b. Non-standard components are used.
- c. The user has not used the device in accordance with the indications for use or the instructions provided in this manual.
- d. The serial number of the apparatus is removed, defaced, misused or altered.
- e. The device, electrodes or batteries are stored or used operationally outside of environmental specifications.
- f. The device has been tested using unapproved methods or inappropriate equipment (see the Maintenance section of this manual).

Any claims made under warranty must be directed via your distributor from whom the device was originally purchased. Before carrying out service under warranty, HeartSine Technologies require evidence of purchase. The product must be used in accordance with the user manual and for the purpose for which it was intended. If you have a query please contact heartsinesupport@stryker.com for assistance.



www.heartsine.com

For further information contact us at heartsinesupport@stryker.com or visit our website at www.heartsine.com.

EMEA/APAC

HeartSine Technologies, Ltd.
203 Airport Road West
Belfast, Northern Ireland
BT3 9ED
Tel: +44 28 9093 9400
Fax: +44 28 9093 9401



U.S./Americas

HeartSine Technologies LLC
121 Friends Lane, Suite 400
Newtown, PA 18940
Toll Free: (866) 478 7463
Tel: +1 215 860 8100
Fax: +1 215 860 8192



©2018 HeartSine Technologies LLC.
All rights reserved.

H017-001-600-6 Intl